



Analysis	Standard Peptide Mass / Purity (HPLC-UV)
Client	Novalabs




Sample

DSIP 10mg
Novalabs

RESULTS

VIAL	BATCH	PURITY	AMOUNT
#1 10mg	May 2026	98.60%	11.25 mg

#1 UV CHROMATOGRAM

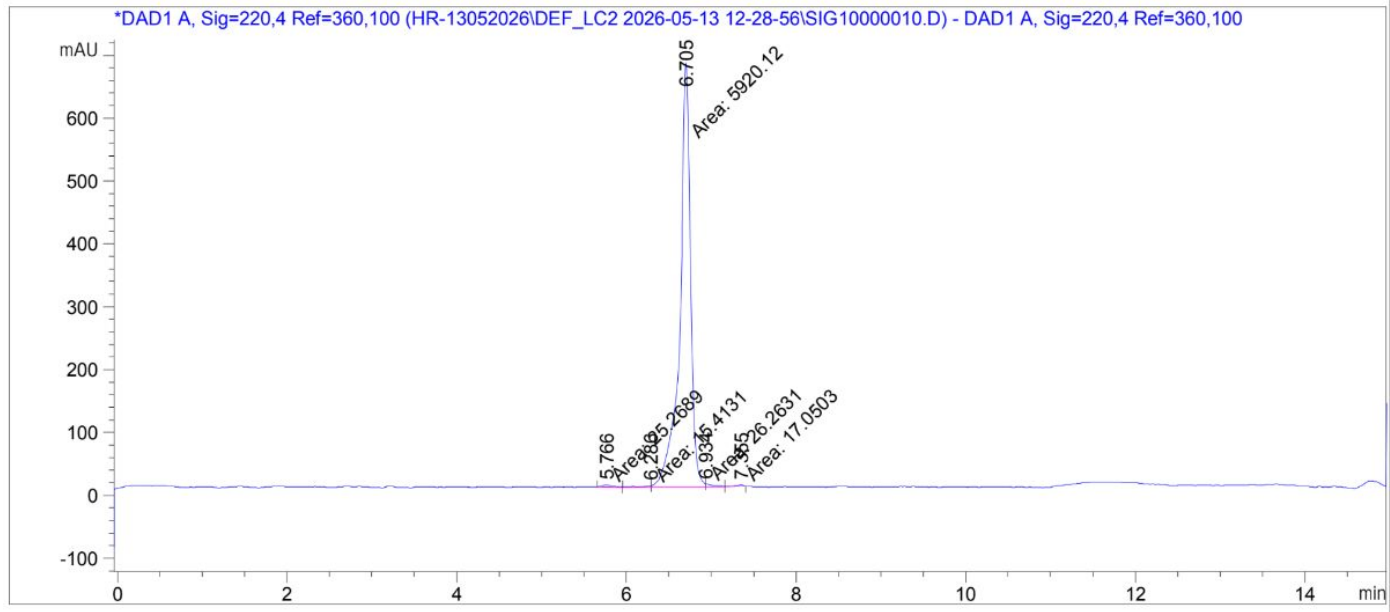

COMMENT

ANALYSIS CONDUCTED
19 MAY 2026
ZAGREB, CROATIA (EU)

Alex Mihaljcic
DIRECTOR

