



Analysis	Standard Peptide Mass / Purity (HPLC-UV)
Client	NovaLabs

Sample


GHK-Cu 50mg
NovaLabs



RESULTS

VIAL	BATCH	PURITY	AMOUNT
#1 50mg	May 2026	99.68%	51.09 mg

#1 UV CHROMATOGRAM

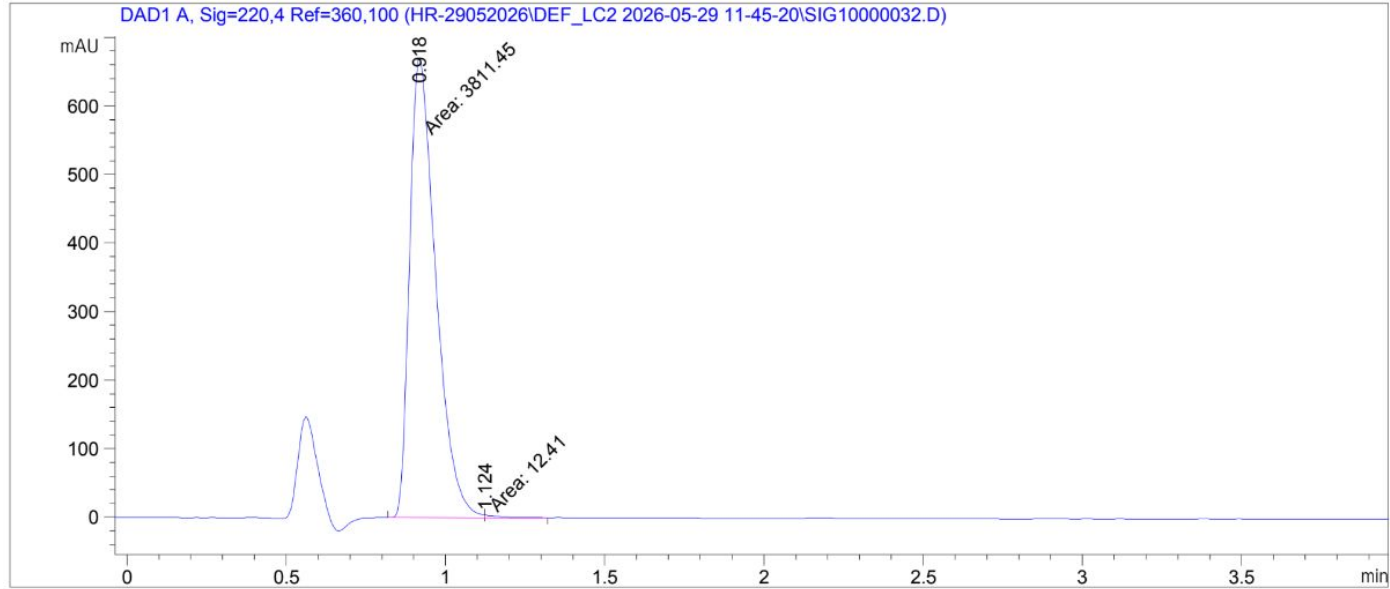

COMMENT

ANALYSIS CONDUCTED

28 MAY 2026

ZAGREB, CROATIA (EU)

Alex Mihaljcic
DIRECTOR

