

Analysis	Standard Peptide Mass / Purity (HPLC-UV)
Client	True North Labs

Sample


MOTS-C	10mg
NovaLabs	



RESULTS

VIAL	BATCH	PURITY	AMOUNT
#1	-	98.78%	11.76 mg

#1 UV CHROMATOGRAM

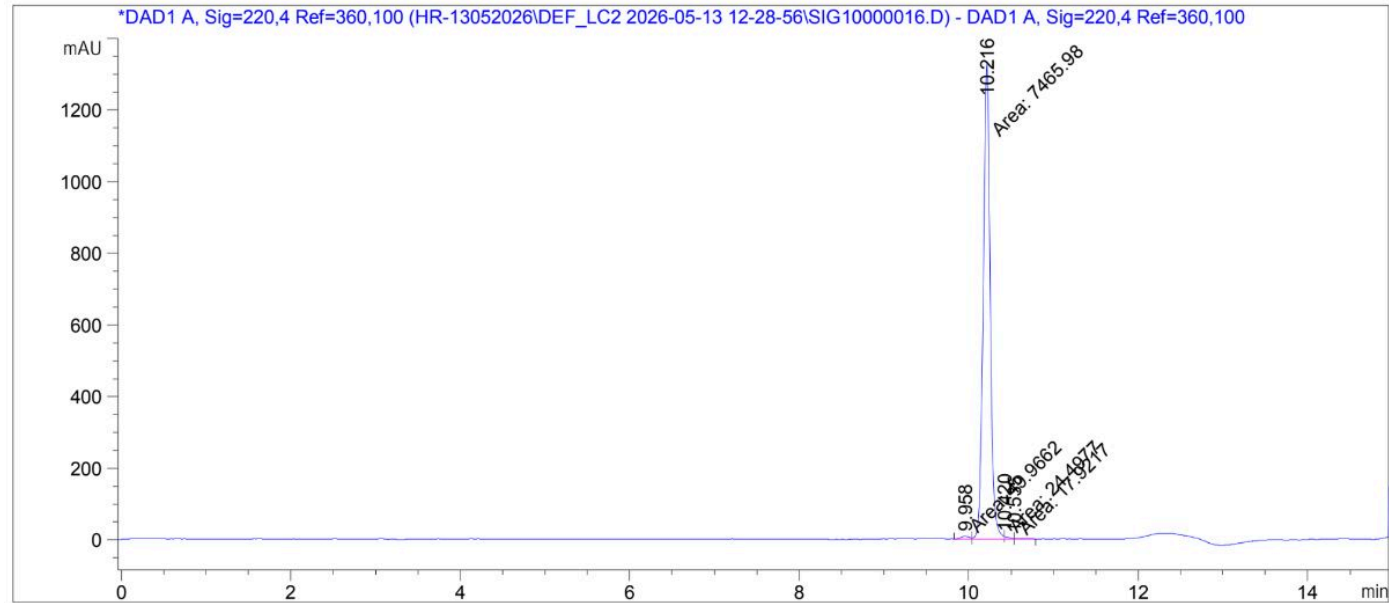

COMMENT

ANALYSIS CONDUCTED

19 MAY 2026

ZAGREB, CROATIA (EU)



Alex Mihaljcic

DIRECTOR

