



Analysis	Standard Peptide Mass / Purity (HPLC-UV)
Client	NovaLabs

Sample


PT-141 10mg
NovaLabs



RESULTS

VIAL	BATCH	PURITY	AMOUNT
#1 10mg	May 2026	99.66%	12.25 mg

#1 UV CHROMATOGRAM

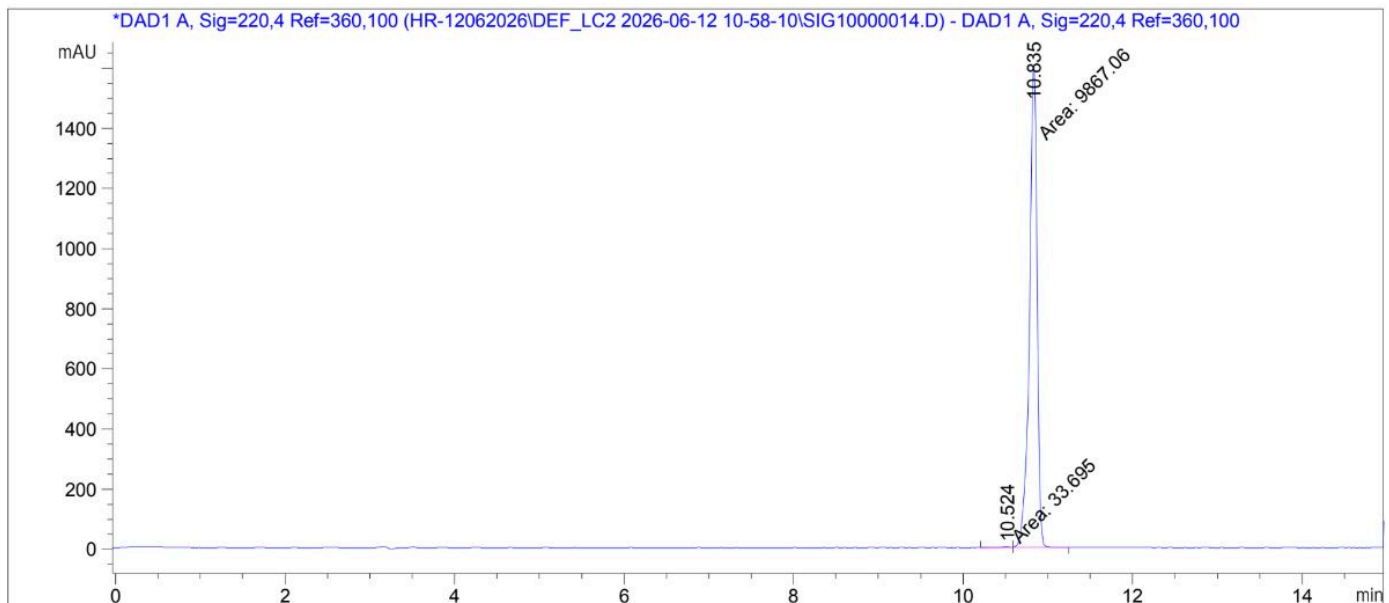

COMMENT

ANALYSIS CONDUCTED

12 JUN 2026

ZAGREB, CROATIA (EU)

Alex Mihaljcic
DIRECTOR