

Analysis	Standard Peptide Mass / Purity (HPLC-UV)
Client	NovaLabs

Sample


Selank 10mg
NovaLabs



RESULTS

VIAL	BATCH	PURITY	AMOUNT
#1 10mg	May 2026	97.99%	12.31 mg

#1 UV CHROMATOGRAM

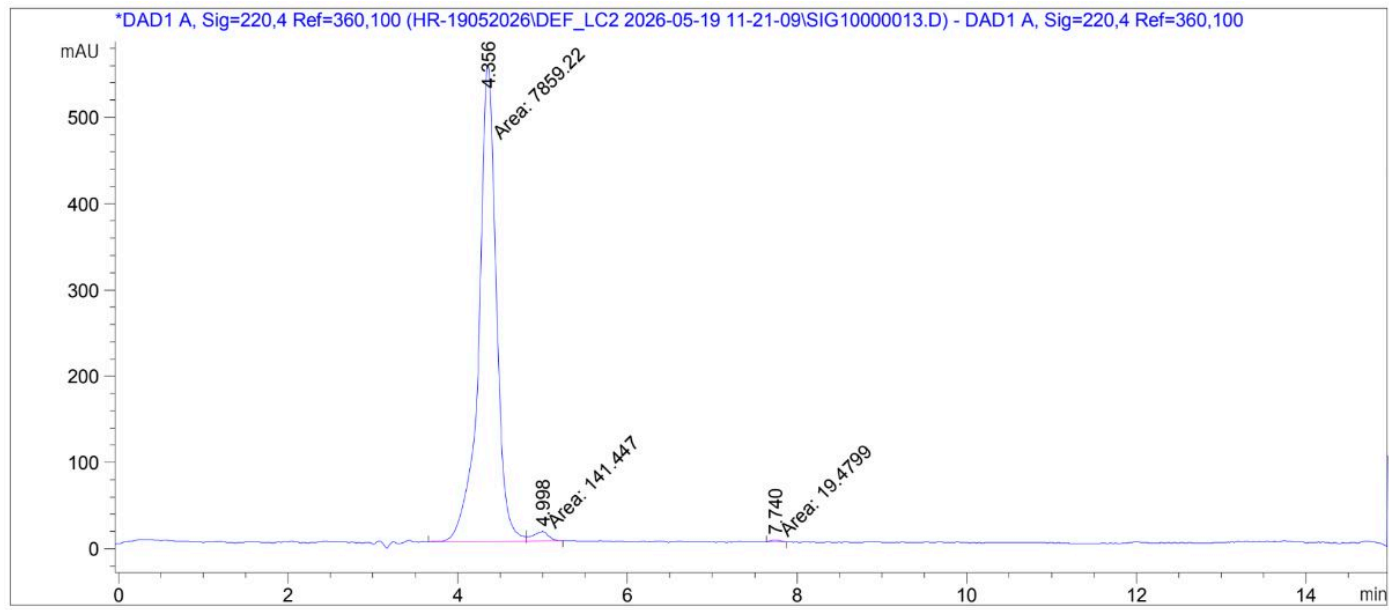

COMMENT

ANALYSIS CONDUCTED

19 MAY 2026

ZAGREB, CROATIA (EU)



Alex Mihaljcic

DIRECTOR

