



Analysis	Standard Peptide Mass / Purity (HPLC-UV)
Client	NovaLabs




Sample

Semax 10mg
NovaLabs

RESULTS

VIAL	BATCH	PURITY	AMOUNT
#1 10mg	May 2026	98.81%	10.79 mg

#1 UV CHROMATOGRAM

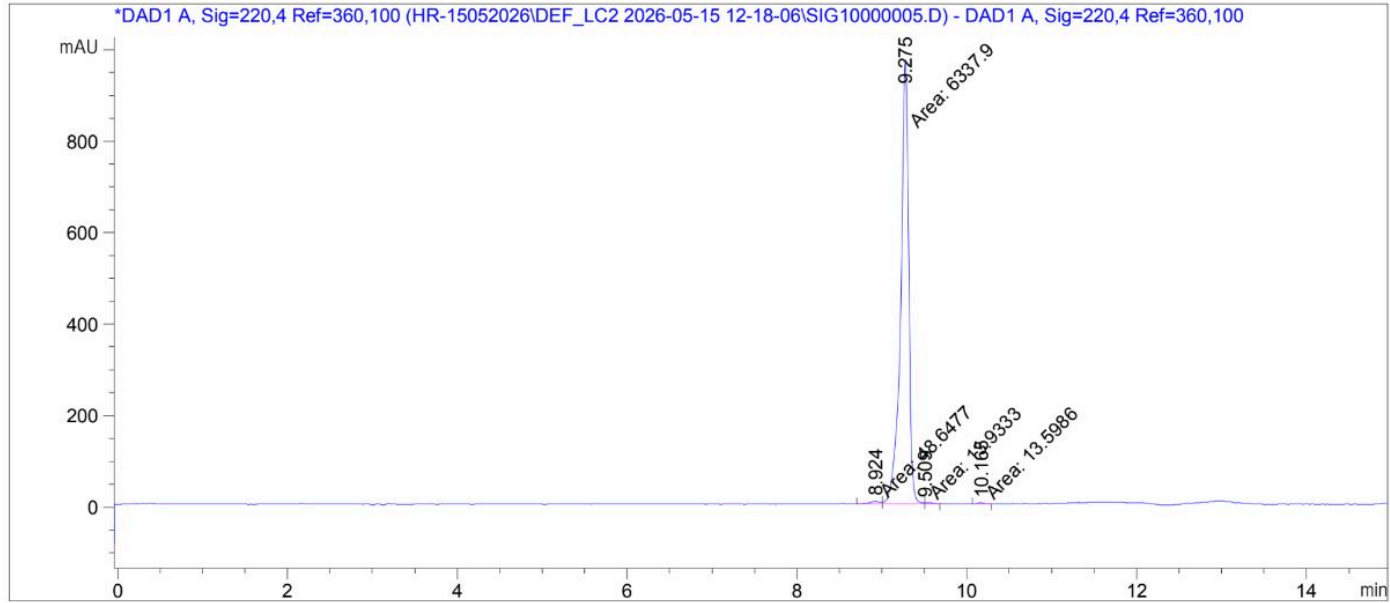

COMMENT

ANALYSIS CONDUCTED

17 MAY 2026

ZAGREB, CROATIA (EU)

Alex Mihaljcic
DIRECTOR

