ANALYSIS REPORT S2M-0DA

Report Generated
07 APR 2026

Analysis	**Standard Peptide Mass / Purity** (HPLC-UV)
Client	NovaLabs

Sample

SS-31 50mg


NovaLabs



RESULTS

VIAL	BATCH	PURITY	AMOUNT
#1 50mg	March	**99.87%**	**49.85** mg

#1 UV CHROMATOGRAM

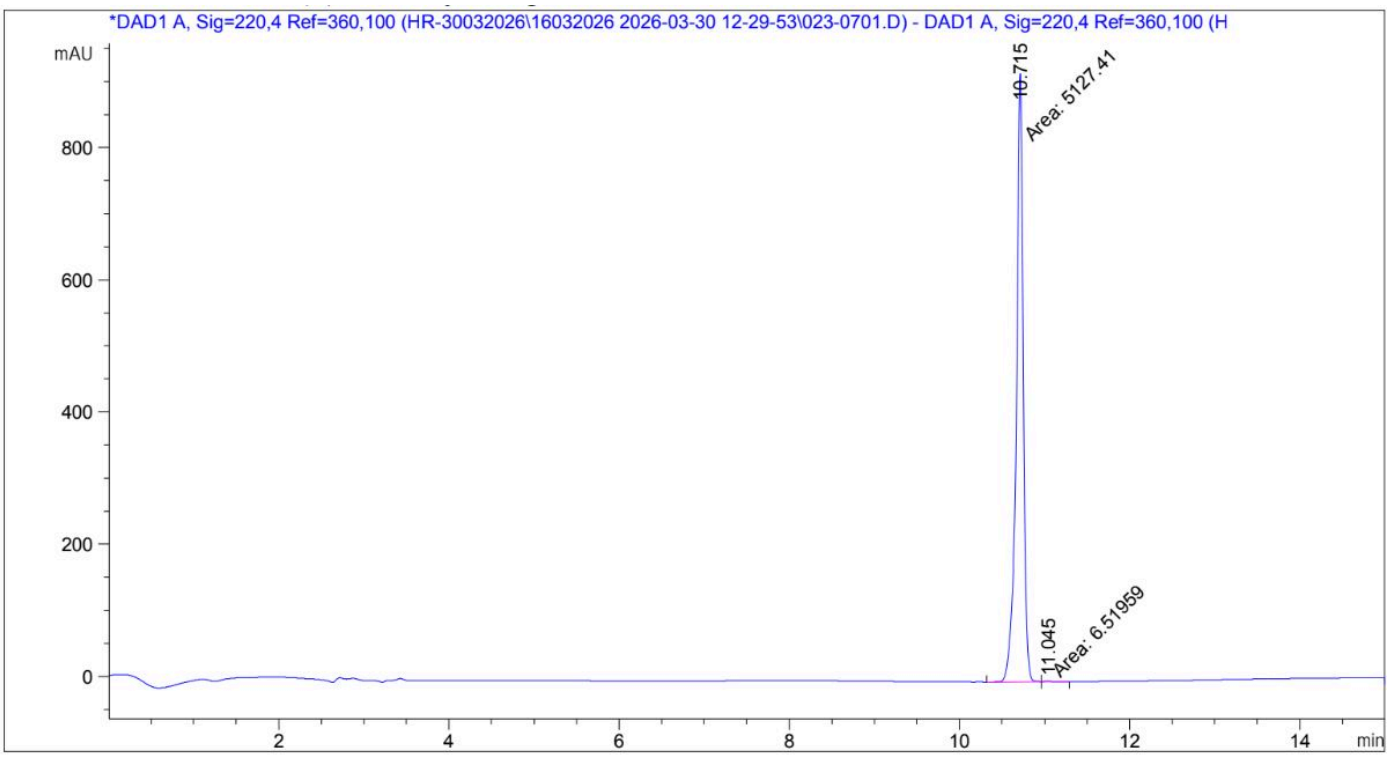

COMMENT

ANALYSIS CONDUCTED

06 APR 2026

ZAGREB, CROATIA (EU)

Alex Mihaljcic
DIRECTOR