

Analysis	Standard Peptide Mass / Purity (HPLC-UV)
Client	NovaLabs

Sample


TB-500	10mg
NovaLabs	



RESULTS

VIAL	BATCH	PURITY	AMOUNT
#1	May 2026	98.44%	10.82 mg

#1 UV CHROMATOGRAM

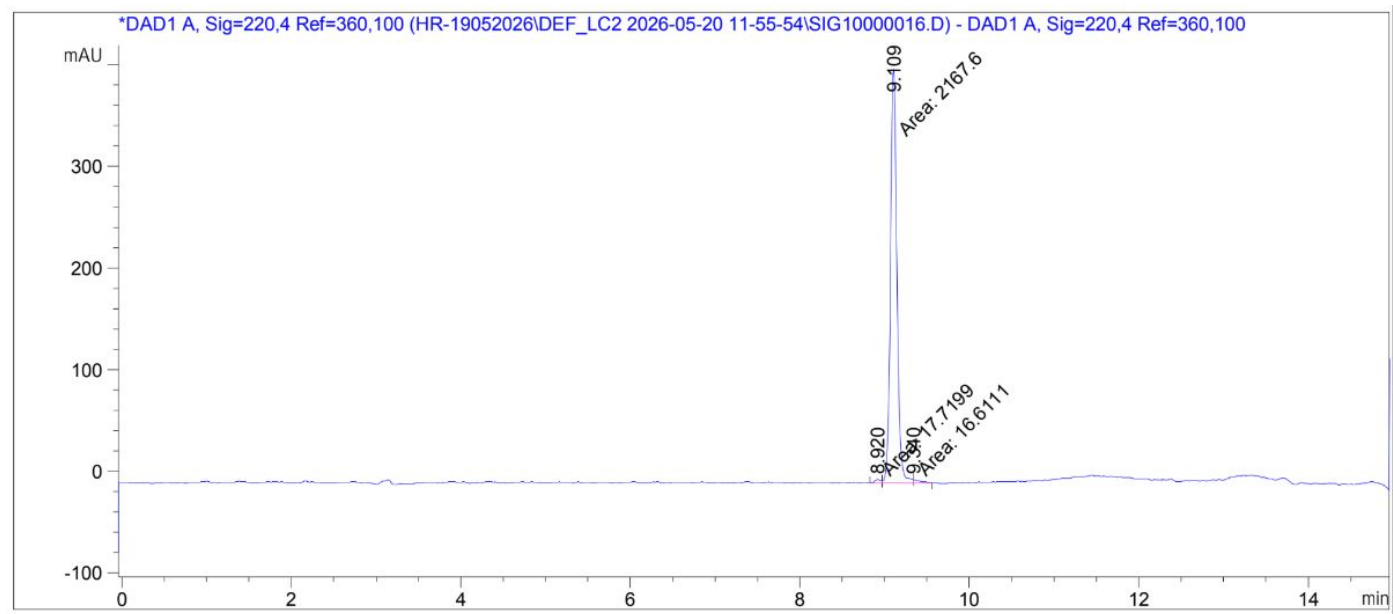

COMMENT

ANALYSIS CONDUCTED

20 MAY 2026

ZAGREB, CROATIA (EU)



Alex Mihaljcic

DIRECTOR

